

APB540Ra61 100µg
Active Cluster Of Differentiation 147 (CD147)
Organism Species: *Rattus norvegicus* (Rat)
Instruction manual

FOR RESEARCH USE ONLY
NOT FOR USE IN CLINICAL DIAGNOSTIC PROCEDURES

12th Edition (Revised in Aug, 2016)

[PROPERTIES]

Source: Eukaryotic expression.

Host: 293F cell

Residues: Ala22~Arg324

Tags: N-terminal His-tag

Purity: >95%

Traits: Freeze-dried powder

Endotoxin Level: <1.0EU per 1µg (determined by the LAL method).

Buffer Formulation: PBS, pH7.4, containing 5% trehalose.

Original Concentration: 200µg/mL

Applications: Cell culture; Activity Assays.

(May be suitable for use in other assays to be determined by the end user.)

Predicted isoelectric point: 4.9

Predicted Molecular Mass: 34.6kDa

Accurate Molecular Mass: 44-55kDa as determined by SDS-PAGE reducing conditions.

Phenomenon explanation:

The possible reasons that the actual band size differs from the predicted are as follows:

1. Splice variants: Alternative splicing may create different sized proteins from the same gene.
2. Relative charge: The composition of amino acids may affects the charge of the protein.
3. Post-translational modification: Phosphorylation, glycosylation, methylation etc.
4. Post-translation cleavage: Many proteins are synthesized as pro-proteins, and then cleaved to give the active form.

5. Polymerization of the target protein: Dimerization, multimerization etc.

[USAGE]

Reconstitute in 10mM PBS (pH7.6) to a concentration of 0.1-1.0 mg/mL. Do not vortex.

[STORAGE AND STABILITY]

Storage: Avoid repeated freeze/thaw cycles.

Store at 2-8°C for one month.

Aliquot and store at -80°C for 12 months.

Stability Test: The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

[SEQUENCE]

```
AAGFLKAPM SQEQWAGGSV VLHCEAVGSP
MPEIQWWFEG NEPNDSQSQL WDGARLDRVH IHATYRQHAA STLSVDGLAA
EDTGTyecra SSDPDRNHLT RPPRVKwvra QASVVVLEPG TIVTSVQEVd
SKTQLTCFLN SSGIDIVGHR WMRGgkvlqe DTLpdlQmky TVDADDRSGE
YSCIFLPEPV GRGNINVEGP PRIKVGKKSE HASEGEFVKL ICKSEASHPP
VDEWVWFKTS DTGDQTIENG TEANSKYVII STPELSELII SLDLMMNVDPG
TYVCNATNSQ GSARETISLR VRSR
```

[ACTIVITY]

Extracellular matrix metalloproteinase (MMP) inducer (EMMPRIN), also known as basigin and CD147, is a 44-66 kDa, variably N- and O-glycosylated, type I transmembrane protein that belongs to the immunoglobulin superfamily. Human EMMPRIN is 269 amino acids (aa) in length and contains a 24 aa signal sequence, a 183 aa extracellular domain (ECD), a 21 aa transmembrane (TM) segment and a 41 aa cytoplasmic tail. The ECD contains one C2-type and one V-type Ig-like domain. EMMPRIN is expressed in areas of tissue remodeling, including endometrium, placenta, skin, and regions undergoing angiogenesis.

It is also expressed on cells with high metabolic activity, such as lymphoblasts, macrophages and particularly tumor cells. A functional ELISA assay was conducted to detect the interaction of recombinant rat EMMPRIN/CD147 and Spike glycoprotein . Briefly, biotin-linked CD147 were diluted serially in PBS, with 0.01% BSA (pH 7.4). Duplicate samples of 100 μ l were then transferred to Spike glycoprotein-coated microtiter wells and incubated for 1h at 37 $^{\circ}$ C . Wells were washed with PBST 3 times and incubation with Streptavidin-HRP for 30min, then wells were aspirated and washed 5 times. With the addition of substrate solution, wells were incubated 15-25 minutes at 37 $^{\circ}$ C . Finally, add 50 μ l stop solution to the wells and read at 450nm immediately. The binding activity of CD147 and Spike glycoprotein was shown in Figure 1, the EC₅₀ for this effect is 0.343 μ g/mL.

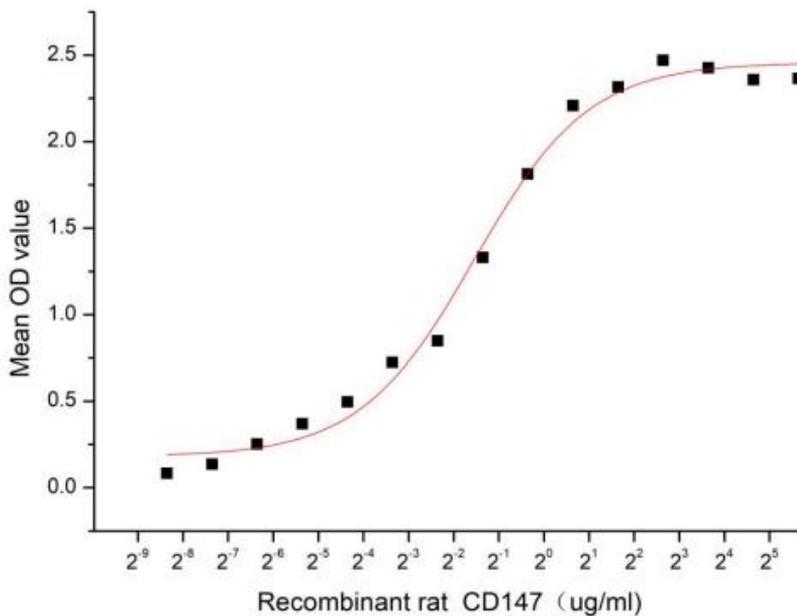


Figure 1. The binding activity of recombinant rat CD147 and Spike glycoprotein

[IDENTIFICATION]

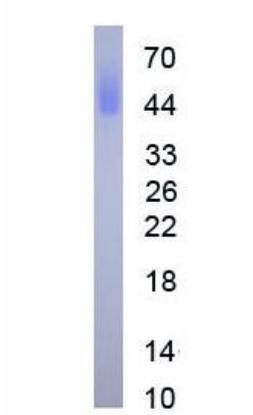


Figure 2. SDS-PAGE

Sample: Active recombinant CD147, Rat

[IMPORTANT NOTE]

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.