

Product Datasheet

Beta-Crosslaps (bCTx) Matched Antibody Pair Kit PSA892Hu11 (96T x 10)

[Products overview]

Matched Antibody Pair Kit is composed of unlabeled capture antibody, Biotinylated competitor and a calibrated peptide / small molecule standard. The Matched Antibody Pair Kit can potentially be used for quantifying natural Beta-Crosslaps (bCTx) in ELISA, CLIA, ELISPOT, Luminex, Immunochromatography and other immunoassays. The Standard in the kit is natural bCTx . Capture antibody is rabbit polyclonal antibody, while Biotinylated competitor is bCTx and BSA coupling complexes.

[Components And Properties]

Components	Quantity	Form
Standard	200ng	Lyophilized, 1 vial
Capture Antibody	500µg / 0.88mL	Liquid, 1 vial, contains 0.1% sodium azide
Biotinylated Competitor	10µg / 0.2mL	Liquid, 1 vial, contains 0.1% sodium azide

Notes: The kit contains raw materials for approximately 96 Tests x 10 plates. However, individual results may vary depending on the researcher's assay protocol and other variables.

[Recommended Buffers and Solutions]

Cloud-Clone's product of Assay Kit Antibody Pairs Support Pack 2 (Cat # IS078), which

includes Coating Buffer, Blocking Buffer, Standard Diluent, Biotinylated Competitor Diluent, Streptavidin-HRP Diluent, Wash Buffer, Streptavidin-HRP, Substrate Solution, Stop Solution is highly recommended for reagent preparation.

[Recommended Range / Dilution]

Standard: Reconstitute the Standard with 1.0mL of Standard Diluent (Cat # IS078). The recommended Range of Standard curve is 98.77 - 8,000pg/mL.

Capture Antibody: Dilute 125 times with Coating Buffer (Cat # IS078). For example, to make enough for 1 plate, add 80uL capture antibody to 9.92mL Coating Buffer.

Biotinylated Competitor: Dilute 550 times with Biotinylated Competitor Diluent (Cat # IS078). For example, to make enough for 1 plate, add 19uL Biotinylated Competitor to 10.431mL Antibody Dilution Buffer.

Notes: The recommended Cloud-Clone's products of diluents and buffers are validated in the lab, other reagents selected for use can alter the performance of an immunoassay.


[Storage]

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -20°C for 12 months. Please make all solutions fresh before the experiment.

Notes: Please avoid contamination.

[Typical Data]

Typical standard curve below is provided for reference only. A standard curve should be generated for each experiment.

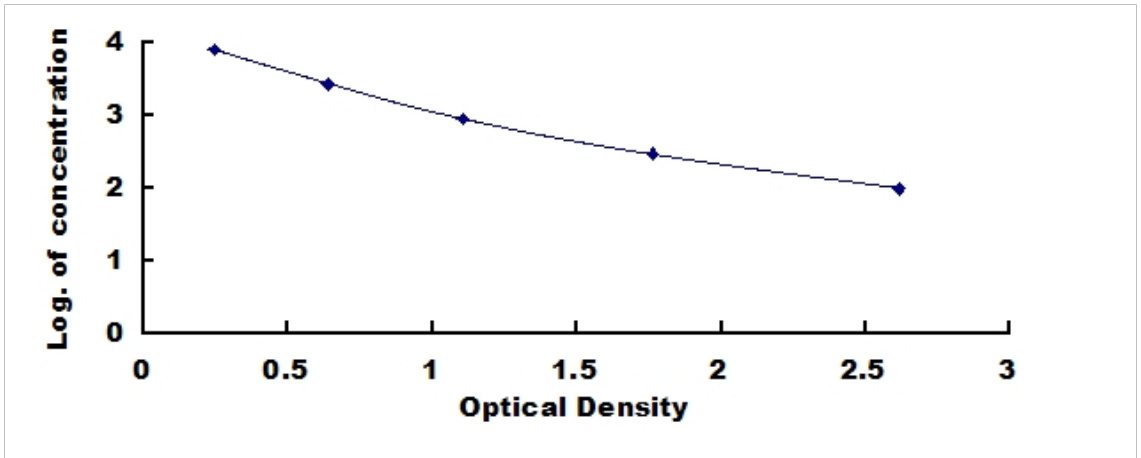

[Recommended Assay Protocol]

1. Dilute the Capture Antibody to working concentration in Coating Buffer. Immediately coat the 96-well microplates with 100 μ L per well of the diluted Capture Antibody. Seal the plate and incubate overnight at 4°C or incubate at 37°C for 2 hours.
2. Aspirate wells and wash with 350 μ L of Wash Buffer (Cat # IS078) per well, and let it sit for 1~2 minutes. Remove the remaining liquid by inverting and tapping the plate on absorbent paper.
3. Block plate with 200 μ L per well of Blocking Buffer (Cat # IS078) for 1.5 hours at 37°C .
4. Repeat the aspiration/wash process as in Step 2.
5. Add 50 μ L of different concentrations of standards, samples into the appropriate wells. And then add 50 μ L of working solution of Biotinylated Competitor to each well immediately. Shake the plate gently (using a microplate shaker is recommended). Cover with the Plate sealer. Incubate for 1 hour at 37°C.
6. Repeat the aspiration/wash process as in Step 2.

7. Add 100 μ L of working solution of Streptavidin-HRP (Cat # IS078) to each well, cover the wells, and incubate for 30 minutes at 37°C.
8. Repeat the aspiration/wash process for total 5 times as in Step 2.
9. Add 90 μ L of Substrate Solution (Cat # IS078) to each well. Cover the wells, and incubate for 10 - 20 minutes at 37°C. Protect from light.
10. Add 50 μ L of Stop Solution (Cat # IS078) to each well. Mix the liquid by tapping the side of the plate.
11. Run the microplate reader and conduct measurement at 450nm immediately.