

Product Datasheet

Human PDL1 Matched Antibody Pair Kit PSA788Hu01

[**Products overview**]

Matched Antibody Pair Kit is composed of unlabeled capture antibody, Biotinylated detection antibody and a calibrated protein standard. The Matched Antibody Pair Kit can potentially be used for quantifying natural and recombinant human Programmed Cell Death Protein 1 Ligand 1 (PDL1) in ELISA, CLIA, ELISPOT, Luminex, Immunochromatography and other immunoassays. The Standard in the kit is recombinant PDL1 . Both capture and detection antibody are rabbit polyclonal antibodies.

[**Components And Properties**]

Components	Quantity	Form
Standard	50µg	Lyophilized, 1 vial
Capture Antibody	200µg / 0.06mL	Liquid, 1 vial, contains 0.1% sodium azide
Biotinylated Detection Antibody	500µg / 1.15mL	Liquid, 1 vial, contains 0.1% sodium azide

[**Recommended Buffers and Solutions**]

Cloud-Clone's product of Assay Kit Antibody Pairs Support Pack 1 (Cat # IS077), which includes Coating Buffer, Blocking Buffer, Standard Diluent, Detection Antibody Diluent, Streptavidin-HRP Diluent, Wash Buffer, Streptavidin-HRP, Substrate Solution, Stop Solution is highly recommended for reagent preparation.


[Storage]

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -20°C for 12 months. Please make all solutions fresh before the experiment.

Notes: Please avoid contamination.

[Typical Data]

Typical standard curve below is provided for reference only. A standard curve should be generated for each experiment.

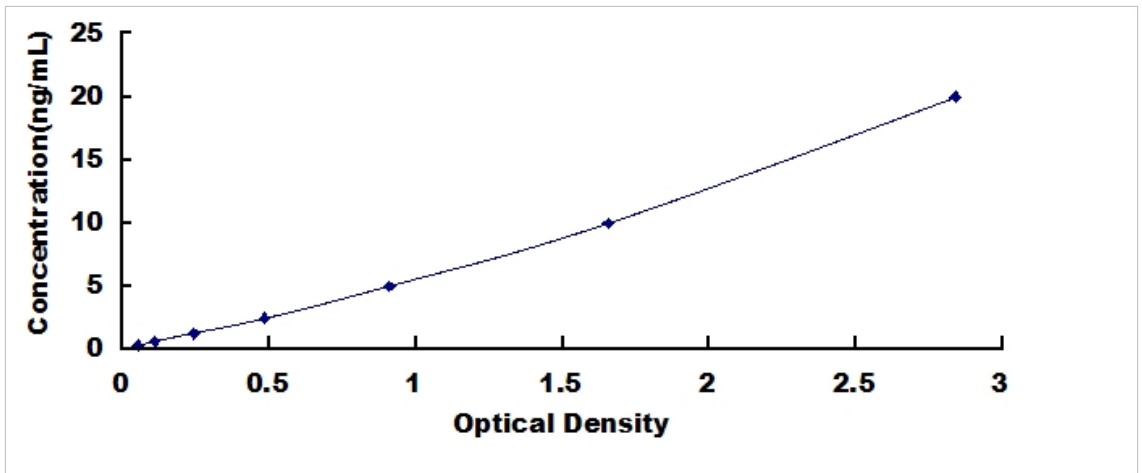

[Recommended Assay Protocol]

1. Dilute the Capture Antibody to working concentration in Coating Buffer. Immediately coat the 96-well microplates with 100µL per well of the diluted Capture Antibody. Seal the plate and incubate overnight at 4°C or incubate at 37°C for 2 hours.

2. Aspirate wells and wash with 350 μ L of Wash Buffer (Cat # IS077) per well, and let it sit for 1~2 minutes. Remove the remaining liquid by inverting and tapping the plate on absorbent paper.
3. Block plate with 200 μ L per well of Blocking Buffer (Cat # IS077) for 1.5 hours at 37°C.
4. Repeat the aspiration/wash process as in Step 2.
5. Add 100 μ L of different concentration of standards, samples into the appropriate wells. Cover with the Plate sealer. Incubate for 1 hour at 37°C.
6. Repeat the aspiration/wash process as in Step 2.
7. Add 100 μ L of the working Biotinylated Detection Antibody working solution to each well, cover the wells, and incubate for 1 hour at 37°C.
8. Repeat the aspiration/wash process for 3 times as in Step 2.
9. Add 100 μ L of the working solution of Streptavidin-HRP (Cat # IS077) to each well, cover the wells, and incubate for 30 minutes at 37°C.
10. Repeat the aspiration/wash process for total 5 times as in Step 2.
11. Add 90 μ L of Substrate Solution (Cat # IS077) to each well. Cover the wells, and incubate for 10-20 minutes at 37°C. Protect from light.
12. Add 50 μ L of Stop Solution (Cat # IS077) to each well. Mix the liquid by tapping the side of the plate.
13. Run the microplate reader and conduct measurement at 450nm immediately.