

RPB091Hu01 50µg

Recombinant Alkaline Phosphatase, Tissue-nonspecific (ALPL)

Organism Species: *Homo sapiens (Human)*

Instruction manual

FOR RESEARCH USE ONLY

NOT FOR USE IN CLINICAL DIAGNOSTIC PROCEDURES

13th Edition (Revised in Aug, 2023)

[PROPERTIES]

Source: Prokaryotic expression

Host: *E.coli*

Residues: Leu18~Arg335

Tags: N-terminal His Tag

Subcellular Location: Membrane

Purity: > 95%

Traits: Freeze-dried powder

Buffer formulation: 20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 0.01% SKL, 5% Trehalose and Proclin300.

Original Concentration: 200µg/mL

Applications: Positive Control; Immunogen; SDS-PAGE; WB.

(May be suitable for use in other assays to be determined by the end user.)

Predicted isoelectric point: 7.0

Predicted Molecular Mass: 39.3kDa

Accurate Molecular Mass: 39kDa as determined by SDS-PAGE reducing conditions.

[USAGE]

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL. Do not vortex.

[STORAGE AND STABILITY]

Storage: Avoid repeated freeze/thaw cycles.

Store at 2-8°C for one month.

Aliquot and store at -80°C for 12 months.

Stability Test: The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

[SEQUENCE]

```

LVP  EKEKDPKYWR  DQAQETLKYA  LELQKLNTNV
AKNVIMFLGD  GMGVSTVTAA  RILKGQLHHN  PGEETRLEMD  KFPFVALSKT
YNTNAQVPDS  AGTATAYLCC  VKANEGTVGV  SAATERSRCN  TTQGNEVTSI
LRWAKDAGKS  VGIIVTTRVN  HATPSAAYAH  SADRWDYSDN  EMPPEALSQG
CKDIAYQLMH  NIRDIDVIMG  GGRKYMYPKN  KTDVEYESDE  KARGTRLDGL
DLVDTWKSFK  PRYKHSFIW  NRTELLTLDP  HNVDYLLGLF  EPGDMQYELN
RNNVTDPSLS  EMVVVAIQIL  RKNPKGFFLL  VEGGR
    
```

[IDENTIFICATION]

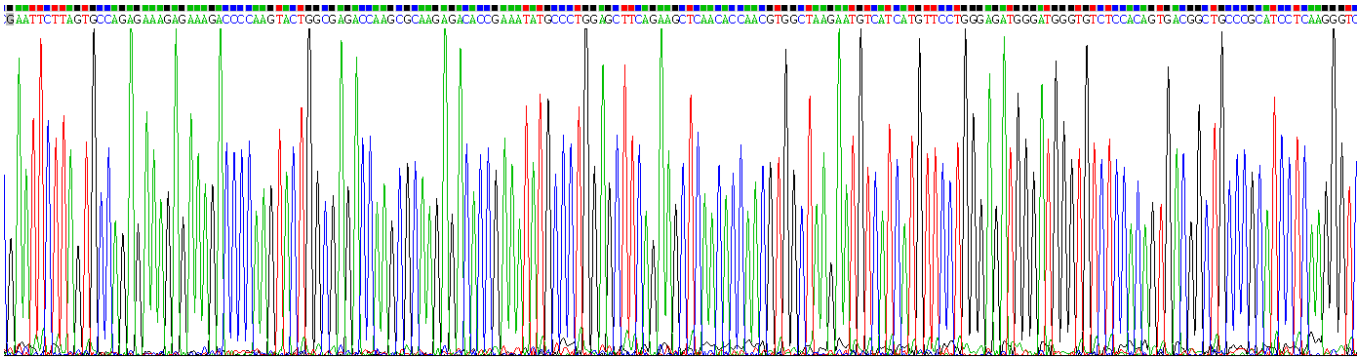


Figure . Gene Sequencing (extract)

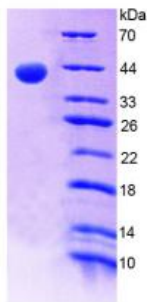


Figure. SDS-PAGE

[IMPORTANT NOTE]

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.