

RPC234Mu01 10µg

Recombinant Cortactin (CTTN)

Organism Species: *Mus musculus* (Mouse)

Instruction manual

FOR RESEARCH USE ONLY

NOT FOR USE IN CLINICAL DIAGNOSTIC PROCEDURES

12th Edition (Revised in Aug, 2016)

[PROPERTIES]

Source: Prokaryotic expression

Host: *E.coli*

Residues: Met1~Gln509

Tags: N-terminal His Tag

Subcellular Location: Cytoplasm

Purity: > 95%

Traits: Freeze-dried powder

Buffer formulation: 20mM Tris, 150mM NaCl, pH8.0, containing 0.01% SKL, 5% Trehalose.

Original Concentration: 200µg/mL

Applications: Positive Control; Immunogen; SDS-PAGE; WB.

(May be suitable for use in other assays to be determined by the end user.)

Predicted isoelectric point: 5.2

Predicted Molecular Mass: 60.7kDa

Accurate Molecular Mass: 75kDa as determined by SDS-PAGE reducing conditions.

Phenomenon explanation:

The possible reasons that the actual band size differs from the predicted are as follows:

1. Splice variants: Alternative splicing may create different sized proteins from the same gene.
2. Relative charge: The composition of amino acids may affect the charge of the protein.
3. Post-translational modification: Phosphorylation, glycosylation, methylation etc.
4. Post-translation cleavage: Many proteins are synthesized as pro-proteins, and then cleaved to give the active form.
5. Polymerization of the target protein: Dimerization, multimerization etc.

[USAGE]

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL. Do not vortex.

[STORAGE AND STABILITY]

Storage: Avoid repeated freeze/thaw cycles.

Store at 2-8°C for one month.

Aliquot and store at -80°C for 12 months.

Stability Test: The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

[**SEQUENCE**]

MWKASAGHAV	SITQDDGGAD	DWETDPDFVN	DVSEKEQRWG	AKTVQGSQHQ	EHINIHKLRE
NVFEHQTLK	EKELETGPKA	SHGYGGKFGV	EQDRMDRSV	GHEYQSKLSK	HCSQVDSVRG
FGGKFGVQMD	RVDQSAVGFE	YQGKTEKHAS	QKDYSSGGFG	KYGVQADRVD	KSAVGFDYQG
KTEKHESQKD	YSKGGGKYG	IDKDKVDKSA	VGFEYQGKTE	KHESQKDYVK	GFGGKFGVQT
DRQDKCALGW	DHQEKLQLHE	SQKDYAKGFG	GKYGVQKDRM	DKNASTFEEV	VQVPSAYQKT
VPIEAVTSKT	SNIRANFENL	AKEREQEDRR	KAEAERAQRM	AKERQEQUEA	RRKLEEQARA
KKQTPPASPS	PQPIEDRPPS	SPIYEDAAPF	KAEPSYRGSE	PEPEYSIEAA	GIPEAGSQQG
LTYTSEPVYE	TTEAPGHYQA	EDDTYGGCES	DLGITAIALY	DYQAAGDDEI	SFDPDDIITN
IEMIDDGWR	GVCKGRYGLF	PANYVELRQ			

[**IDENTIFICATION**]


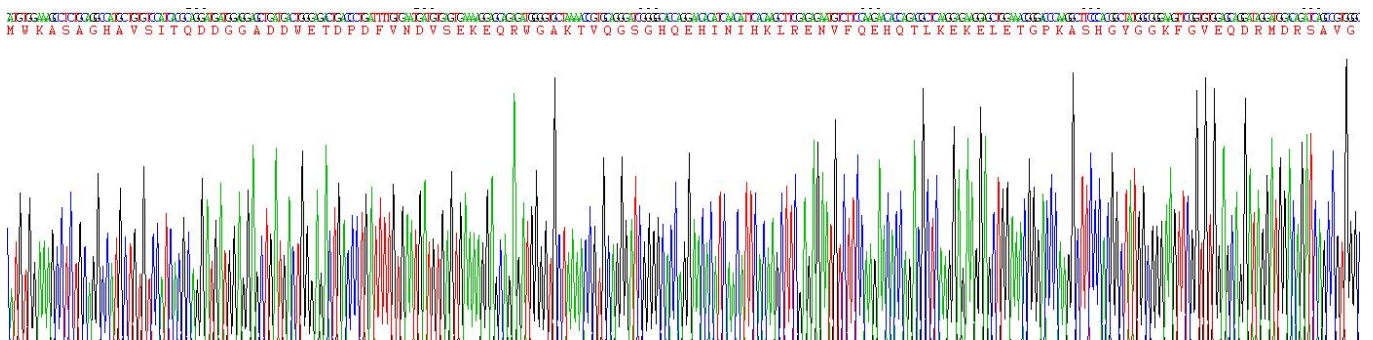


Figure. Gene Sequencing (Extract)

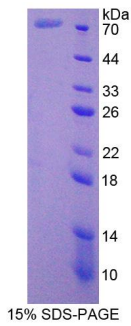

[IMPORTANT NOTE]

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.